




Phonak Virto P-10 NW O (P90/P70/P50/P30)


M Receiver 2 cm³ coupler data

ANSI / ASA S3.22-2014 (R2020)
IEC 60118-0 : 2022

Output sound pressure level

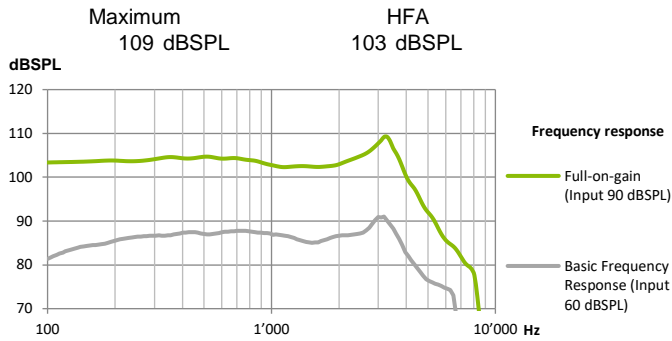


Acoustic gain

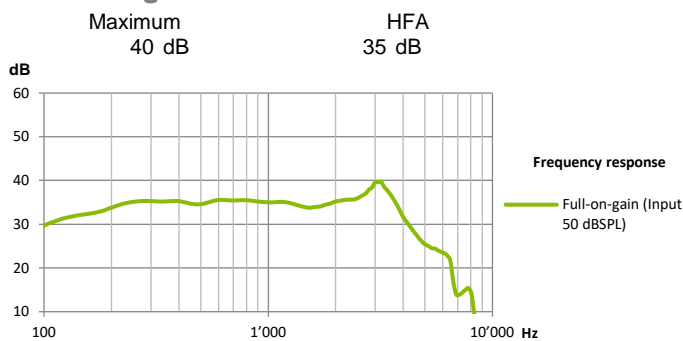

Frequency range	<100 Hz - 7000 Hz			
Total harmonic distortion	500 Hz	800 Hz	1600 Hz	3200 Hz
	1.0%	1.5%	1.0%	1.0%
Battery current	1.1 mA			
Equivalent input noise level	19 dBSPL			


Induction coil sensitivity

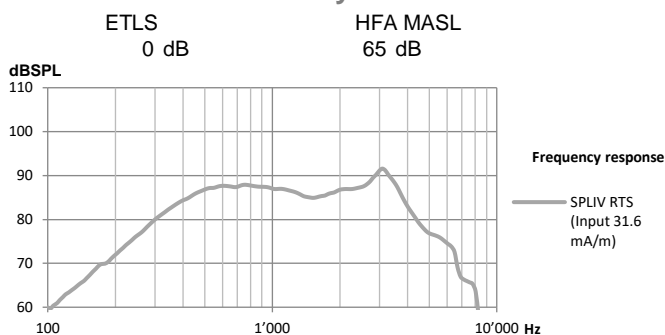


P Receiver 2 cm³ coupler data

ANSI / ASA S3.22-2014 (R2020)
IEC 60118-0 : 2022

Output sound pressure level

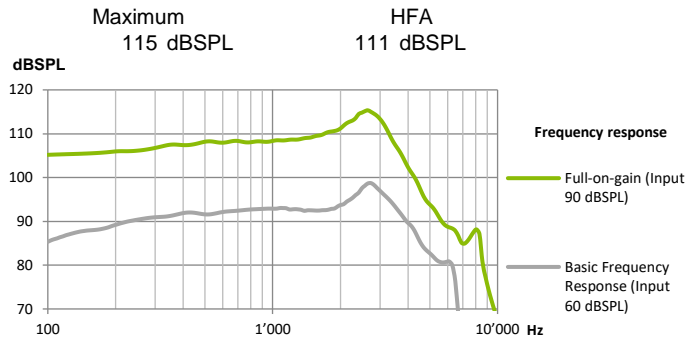


Acoustic gain

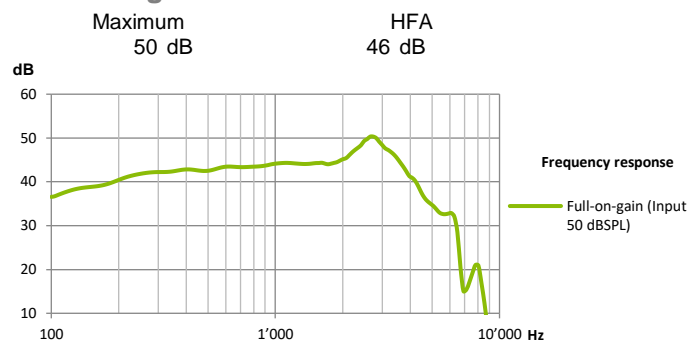

Frequency range	<100 HZ - 6700 Hz			
Total harmonic distortion	500 Hz	800 Hz	1600 Hz	3200 Hz
	1.0%	1.0%	1.0%	1.0%
Battery current	1.2 mA			
Equivalent input noise level	19 dBSPL			

Induction coil sensitivity

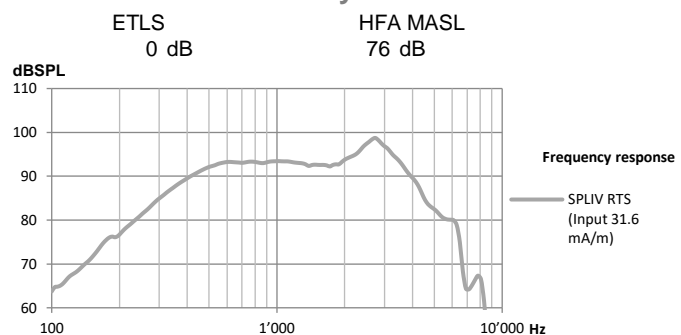

General test information

- Supply voltage 1.3 V / impedance 6.2 Ω
- Specific measurement settings are used. RTS adjustment with volume control
- The device is operating in linear mode
- Low-level expansion is active
- Unless otherwise specified, all data obtained are measured with 5 mm tubing and Phonak Target measurement settings
- The latency of the audio signal determined according an internal standard is 6.2 ms

WARNING: Changes or modifications to the hearing aid that are not explicitly approved by the manufacturer are not permitted.
Such changes may damage the ear or the hearing aid




Phonak Virto P-10 NW O (P90/P70/P50/P30)

SP Receiver


2 cm³ coupler data

ANSI / ASA S3.22-2014 (R2020)
IEC 60118-0 : 2022

Output sound pressure level

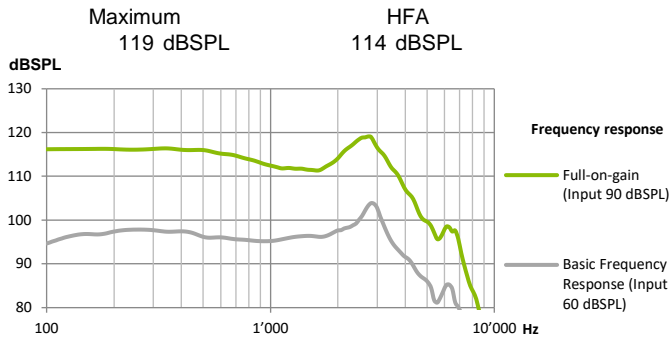


Acoustic gain

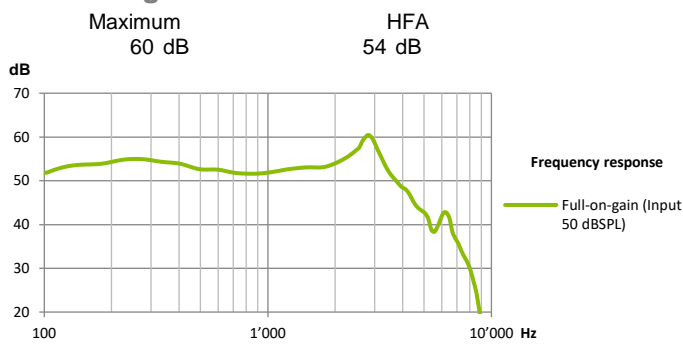

Frequency range	<100 Hz - 7000 Hz			
Total harmonic distortion	500 Hz	800 Hz	1600 Hz	3200 Hz
	1.0%	1.0%	1.0%	1.0%
Battery current	1.1 mA			
Equivalent input noise level	19 dB SPL			

Induction coil sensitivity

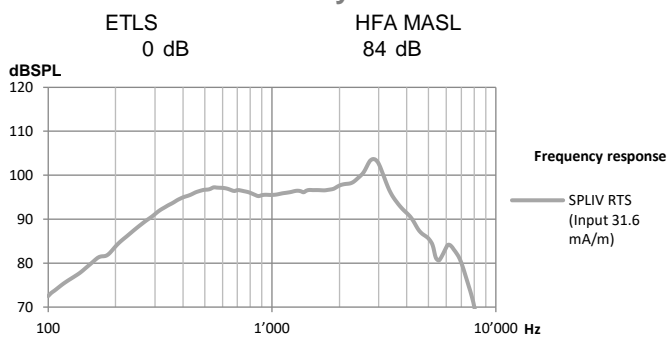

Sonova AG · Laubisrütistrasse 28
CH-8712 Stäfa · Switzerland
www.phonak.com

A Sonova brand

PHONAK
life is on